



HPLC

<Chromatogram>


mV

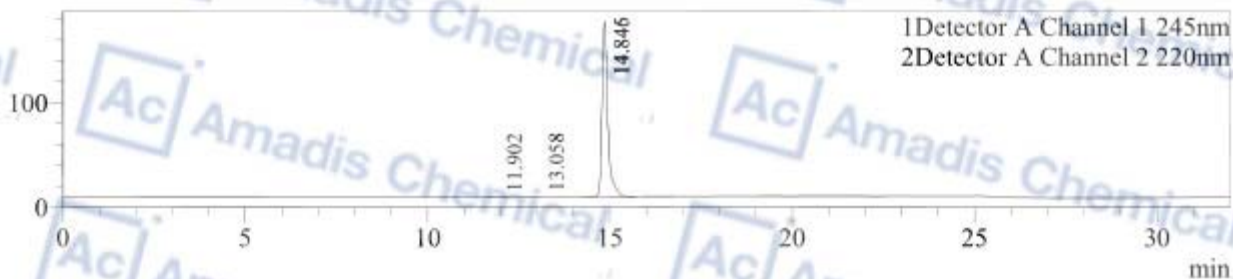

mV

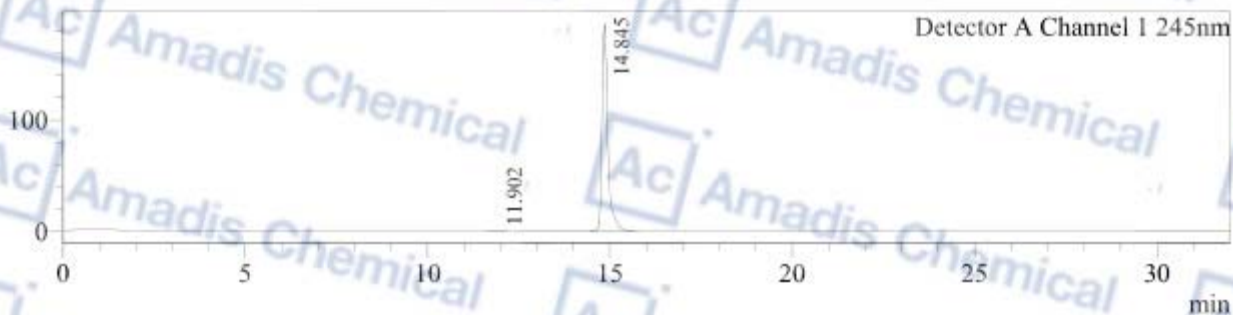

mV

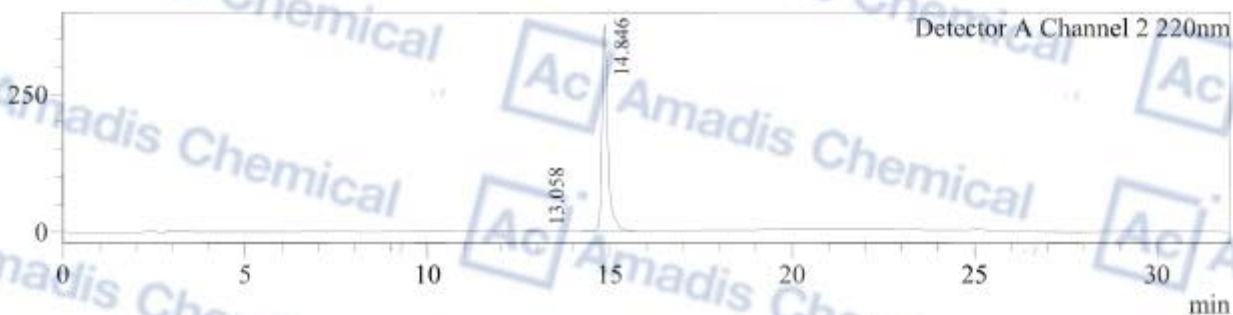

<Peak Table>

Detector A Channel 1 245nm

Peak#	Ret. Time	Area	Area%	Height	Resolution(USP)	Tailing Factor
1	11.902	860	0.043	59	--	1.231
2	14.845	2009055	99.957	186056	9.756	1.623
Total		2009915	100.000	186115		

Detector A Channel 2 220nm

Peak#	Ret. Time	Area	Area%	Height	Resolution(USP)	Tailing Factor
1	13.058	767	0.019	-0	--	--
2	14.846	4078320	99.981	374972	5.998	1.625
Total		4079087	100.000	374972		

***** End Of Report *****