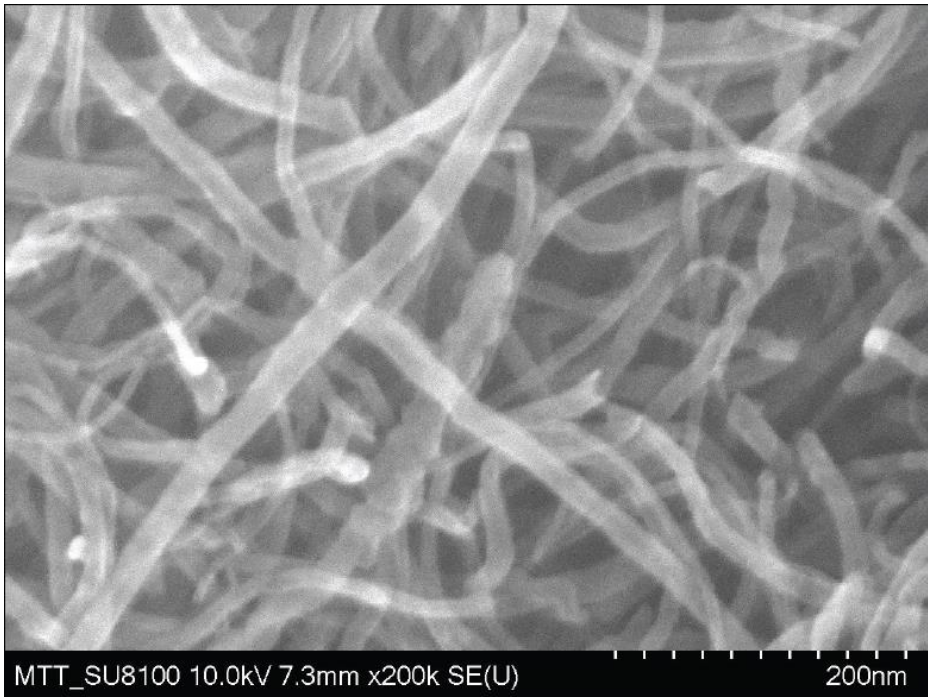


## Certificate Of Analysis

**Name:** Carbon Nanotube  
**CAS No.:** 308068-56-6  
**Cat No.:** A947409  
**Batch No.:** C22072022  
**Mfg.Date:** 2022.07.22  
**Exp.Date:** 2024.07.21

Analytical Technique	Inductively Coupled Plasma/Elemental Analyzer	
<b>Analysis Result</b>	Chemical Composition	Analysis
	Ca	≤0.005%
	Fe	≤0.010%
	Mg	≤0.010%
	Zn	≤0.005%
	Al	≤0.010%
	Mn	≤0.005%
	P	≤0.005%
	Cu	≤0.010%
	S	≤0.005%
	Ni	≤0.010%
	W	≤0.010%
Si	≤0.010%	
Analytical Technique	Malvern NanoZS/ JEM-2010/FEI SIRION-20	

<p>TEM/SEM</p>	
<p><b>Analysis Result</b></p>	<p>Z-AVERAGE=20nm</p>
<p><b>Conclusion</b></p>	<p>The product tested complies with the specifications.</p>

**Storage condition: Store in a tightly closed container in a cool and dry place.**

Checker:

-----  
 \*If you have any comments and suggestions, please contact us by [sales@amadischem.com](mailto:sales@amadischem.com)

\*For laboratory or manufacturing use only, not for drug, food and household use.